

# Maxi Move


## Apply and release brake

Apply break





For storage and on incline only. Do not apply brakes when lifting a patient in any other way.


Release brake

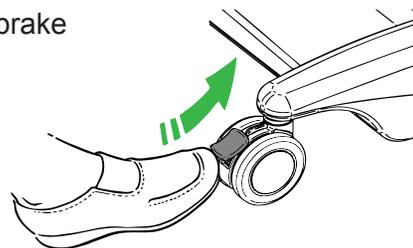


## Control panel and Control handset buttons

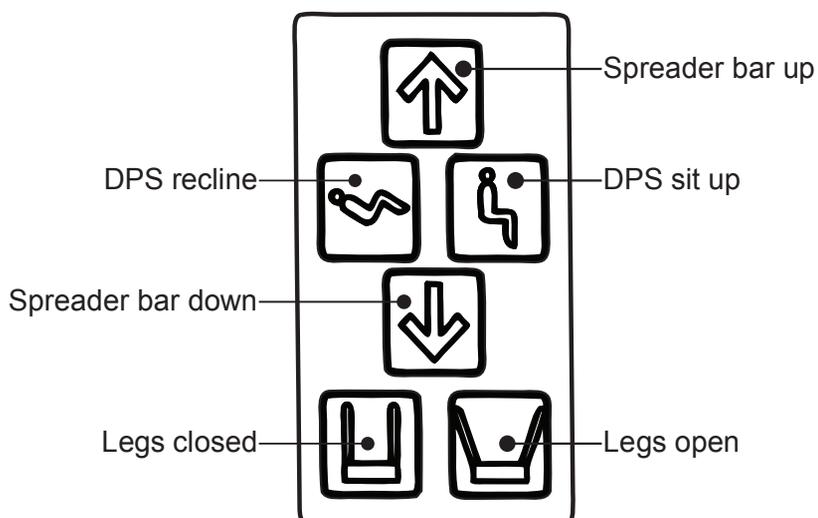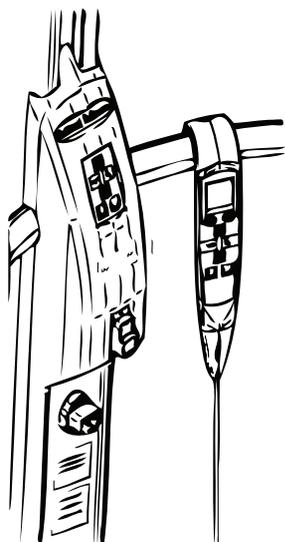




## Loop sling attachment

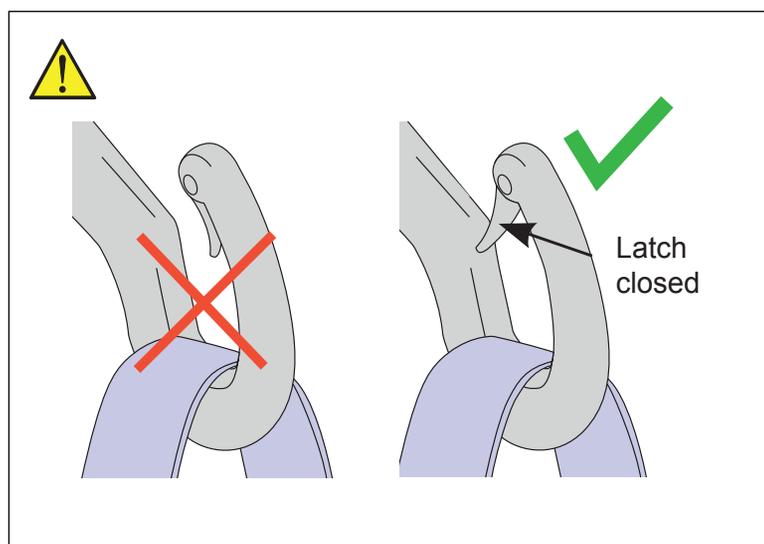




## Clip sling attachment

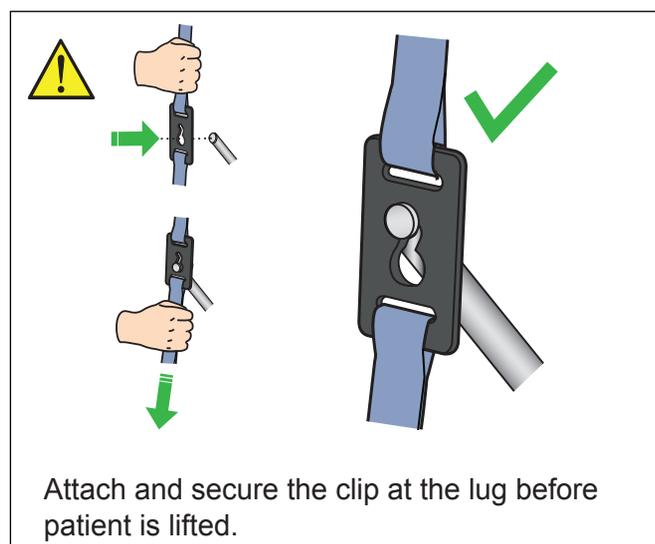

## Remove attachment

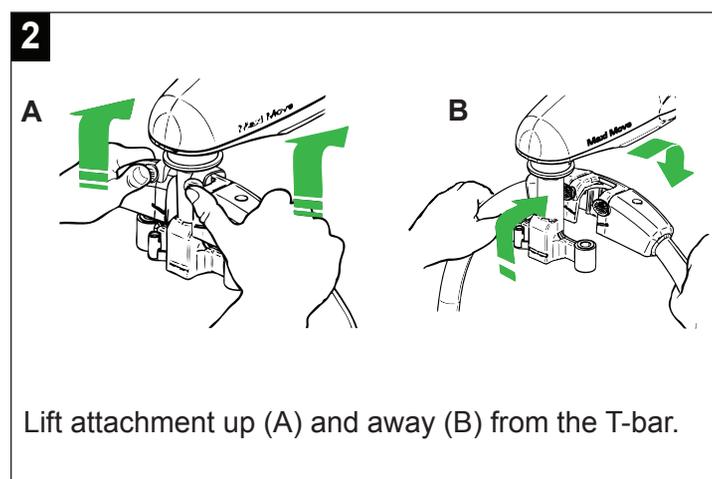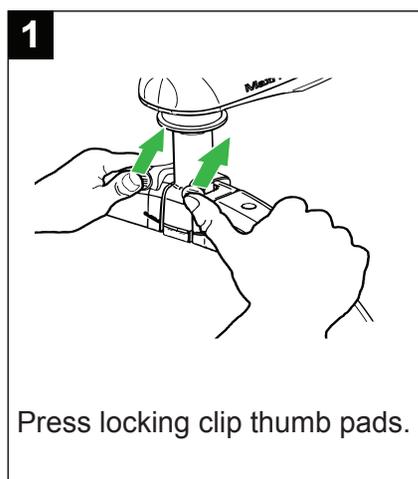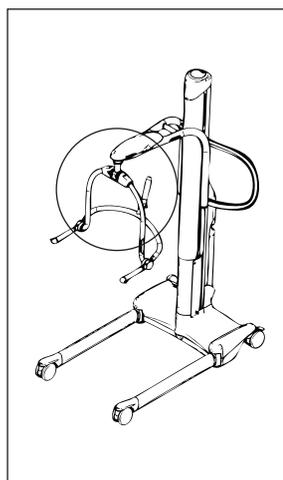

## Install attachment

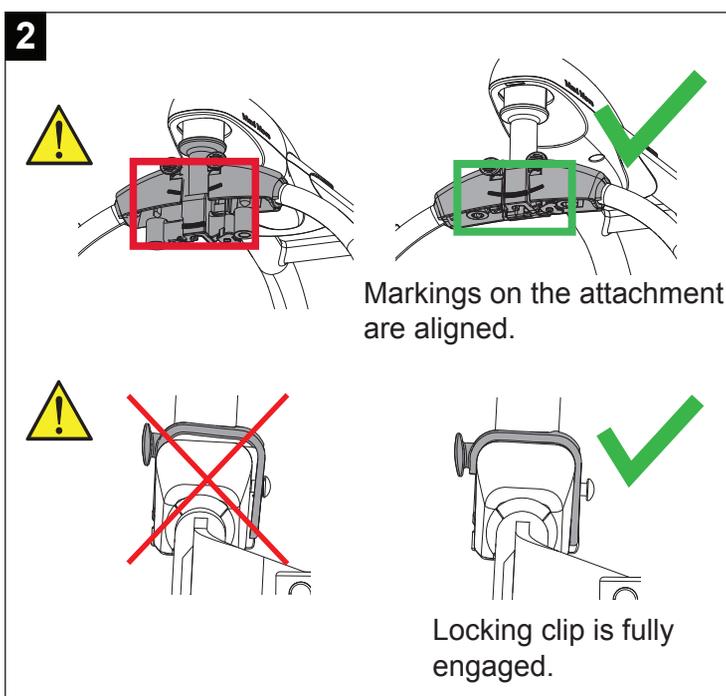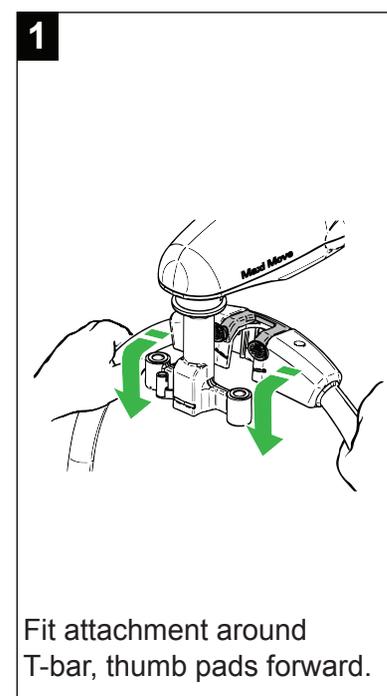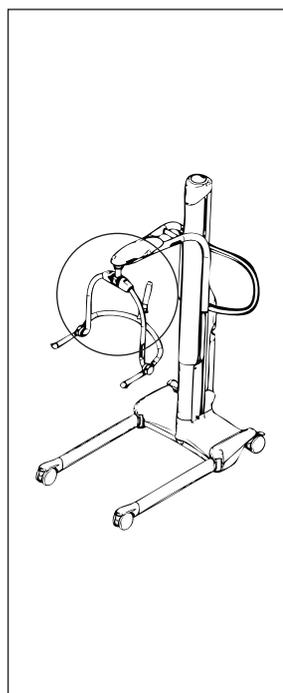

## Electrical power fail – lower the jib

